


# MD Test laboratory – decision rule

Definition for determination of results in the test laboratory:

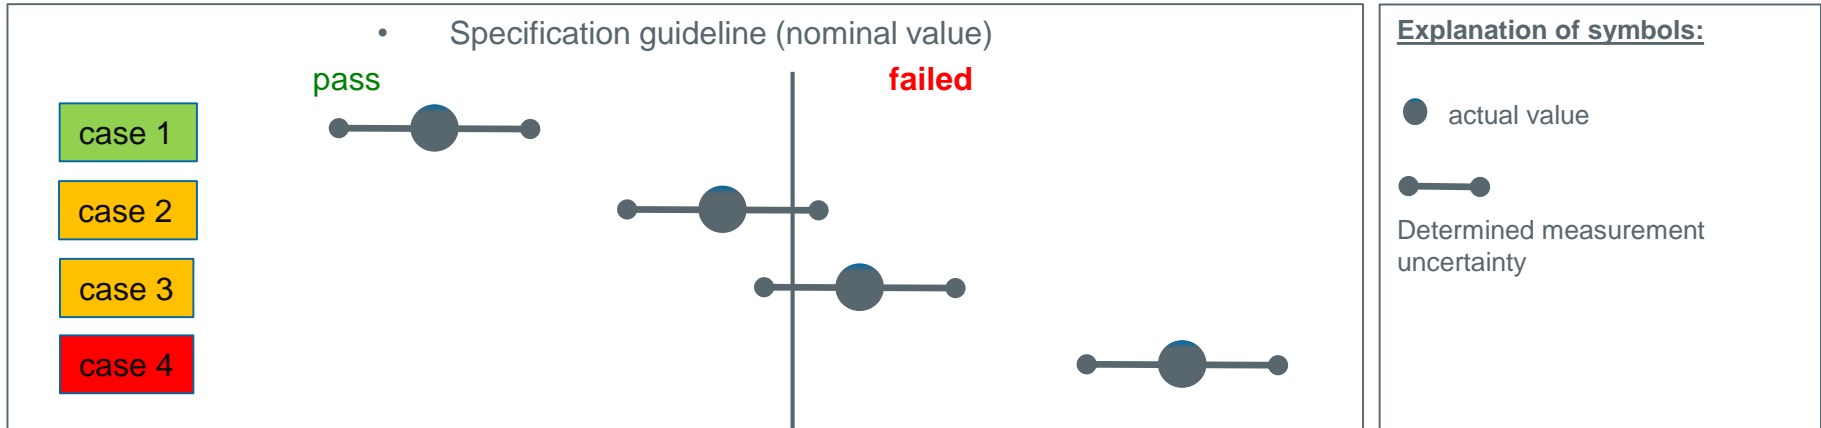

## Description of the cases:

Case 1: Within specification, with measurement uncertainty taken into account

Case 2: The measured value with its confidence interval overlaps the acceptance limit. A clear pass / fail rating is not possible at the required level of significance.

Case 4: Out of specification, with measurement uncertainty take into account